



Ankle Fusion Plating System

The ankle fusion plating system is a new type of polyaxial plating system for ankle arthrodesis. The system provides a complete solution for tibiotalar (TT) and tibiotalocalcaneal (TTC) arthrodesis.

The anatomically adapted plates allow ventral, anterolateral, dorsal or lateral access. The screws can be placed either polyaxially or monoaxially. A clear color-coded instrument set completes the innovative system.

Ankle Fusion Plate TT, anterolateral

Talus fixation due to polyaxial screw holes

Optional temporary fixation with K-Wires

The oblong hole allows axial compression

Compression hole for cannulated screws Ø 7.3 mm

Cortical Screw Ø 4.5 mm
Locking Cancellous Bone Screw Ø 6.5 mm

- Drill Bit Ø 3.2 mm
- Drill Guide 3.2
- Double Drill Guide 3.2 / ML





Locking Cortical Screw Ø 5.0 mm

- Drill Bit Ø 4.2 mm
- Drill Guide 4.2
- Double Drill Guide 4.2 / ML



Cannulated Screw Ø 7.3 mm

- Drill Bit Ø 5.0 mm
- Centering Sleeve 5.0 for K-Wire
- Drill Guide 5.0

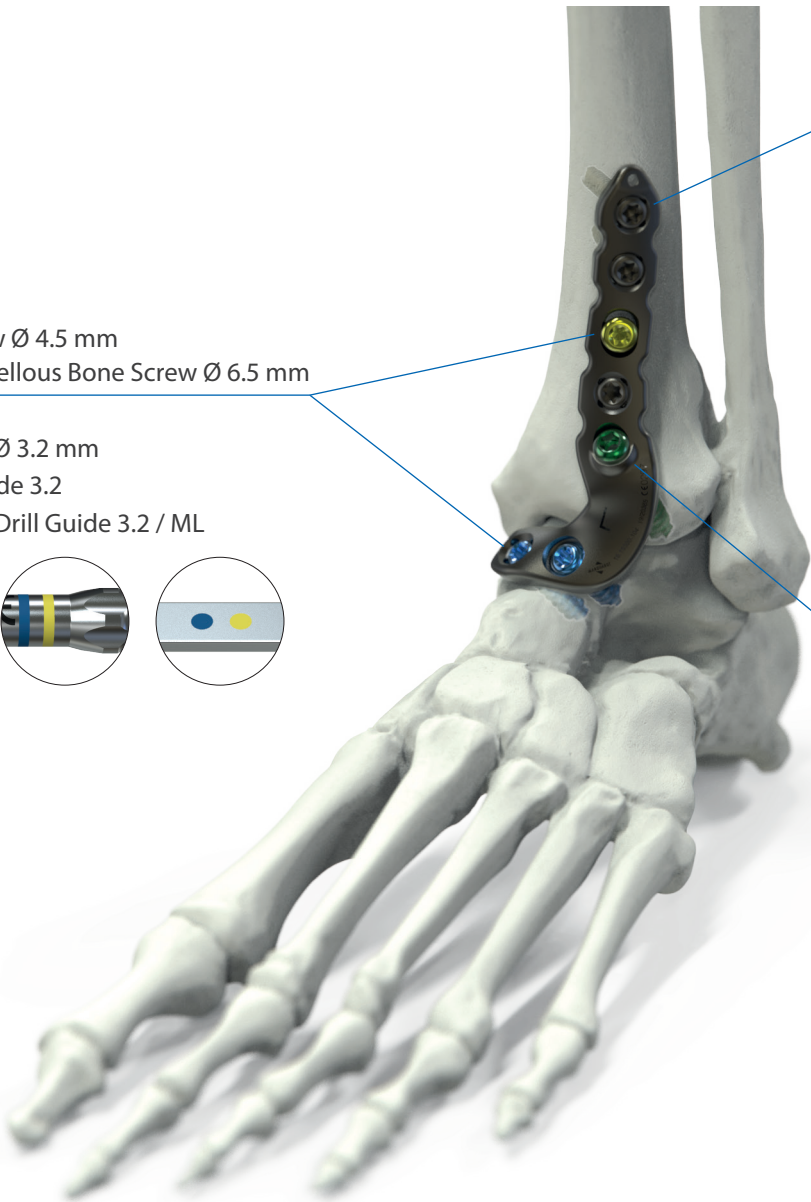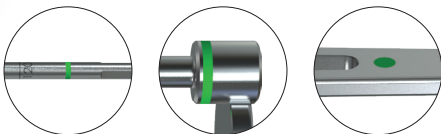

Ankle Fusion Plate TT, anterior

Compression hole for
Ø 7.3 mm transfixation screw

Oblong hole for optional compression

All screw holes can be equipped with
locking or non-locking screws

Ankle Fusion Plate TTC, lateral

Titanium implants with type II anodization

Oblong hole for optional compression

Compression hole for Ø 7.3 mm
transfixation screw


Stable fixation for talus and calcaneus
via 9 polyaxial screw holes

Ankle Fusion Plate TTC, posterior

Compression hole for Ø 7.3 mm
transfixation screw

4 polyaxial screws for secure fixation
in the calcaneus and talus

Ankle Fusion Plating System

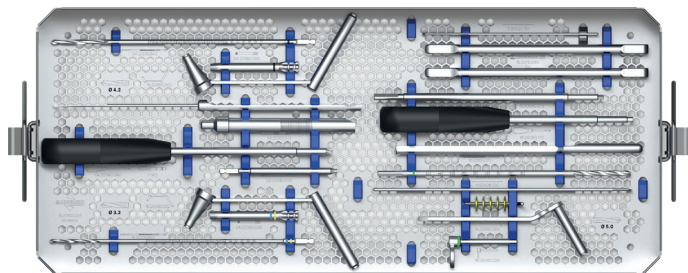

Instruments



Ankle Fusion Plate TT, anterolateral

16.15300.1XX(S) left 16.15300.0XX(S) right

Holes 4, 6

Length 93, 118 mm




Ankle Fusion Plate TT, anterior

16.15350.1XX(S) left 16.15350.0XX(S) right

Holes 3, 5

Length 102, 130 mm




Cortical Screw Ø 4.5 mm, self-tapping

04.03745.XXX Length 20-50 mm



Locking Cortical Screw Ø 5.0 mm, self-tapping

04.05755.XXX Length 20-60 mm



Locking Cancellous Bone Screw Ø 6.5 mm, self-tapping

04.05800.XXX Length 20-60 mm



Ankle Fusion Plate Template

16.15xxx.xxx 1 = Implant

16.25xxx.xxx 2 = Template

Templates are available for all plate types



Ankle Fusion Plate TTC, posterior

16.15200.1XX(S) left 16.15200.0XX(S) right

Holes 3, 5

Length 108, 136 mm



Ankle Fusion Plate TTC, lateral

16.15100.00X(S)

Holes 3, 5

Length 119, 147 mm



Cannulated Ø 7.3 mm, self-tapping

08.03916.XXX Length 45-100 mm



Cannulated Ø 7.3 mm, self-tapping

08.03932.XXX Length 50-100 mm



Cannulated Ø 7.3 mm, self-tapping

08.03900.XXX Length 50-100 mm

You can also find us on social networks:



Note:

This description is not sufficient for immediate application of the instruments. Further information is available in the detailed surgical technique. Maintenance, care and preparation of Marquardt instruments can be found in the corresponding instructions.